

Bettersizer S3 Plus Strive For Excellence In All You See



Strive for Excellence in All You See

The Bettersizer S3 Plus combines laser diffraction and dynamic image analysis in one instrument. It can measure the size and shape of particles from 0.01 µm to 3500 µm. Its exceptional sensitivity for either ultrafine particles or oversized particles, and unsurpassed resolution, make it the most powerful size and shape analyzer for users across various industries, offering new possibilities for comprehensive particle characterization solutions.



Moasurect Lunar Source Source

9

2

BT-803

"The combination of laser diffraction and dynamic image analysis perfectly meets the needs of coarse particle measurement in polymer product development and the results obtained are reliable and highly accurate."

)

BT-A60

 \bigcirc

(I'AN Thermal Power Research Institute Co., Ltd.

Applications and Industries

Industries	Samples	Significance	Industries	Samples
Soils & Sediments	Stones, clay, gravel, marine sediments, lunar surface, etc.	Particle size and shape are two fundamental properties of any sediment or soil that can provide important clues to its nature and origin. The Bettersizer S3 Plus offers accurate and reliable particle size and shape information in the range 0.01-3500 µm for various sample types including soils, marine sediments and even lunar samples returned from space missions.	Battery & Energy	Graphite, cobalt, manganese, etc.
Ceramics	Silica, quartz, flint, silicates, alumina, etc.	The particle size distributions of raw ceramic materials significantly impact the final product's surface smoothness, shapes, degree of agglomeration and dimensional stability. The dual camera optical system in Bettersizer S3 Plus effectively captures the images of agglomerated oversized particles during R&D processes.	Paints, Inks, & Coatings	Epoxies, polyurethanes, silicon, zinc-rich primers, etc.
Abrasives	Calcite, emery, pumice, sandstone, garnet, borazon, etc.	Optimizing particle size and size distribution in abrasive materials maximize final products' performances while minimizing material waste. Monitoring particle size and identifying agglomerations in raw material could be achieved via the dynamic image analysis technology in Bettersizer S3 Plus.	Pharmaceuticals Image: Constraint of the second s	Cefixime, gliclazide, glimepiride, paclitaxel, etc.
3D Printing Materials	Polylactic acid (PLA), Acrylonitrile butadiene styrene (ABS), bronze, nickel, alloy, etc.	The flow property, surface roughness, and quality of 3D printed products greatly depend on its raw material's particle size and size distribution. The Bettersizer S3 Plus helps optimize particle size distribution, thereby controlling the final product's quality.	Building Materials	Cement, asphalt, sands, wood, synthetic polymers, etc.
Food & Beverages	Sugar, chocolate, flour, additives, etc.	Many important characteristics of food products, namely taste, dissolution, and extraction behavior, are affected by particle sizes and shapes of raw materials. Equipped with dynamic image analysis technology, the Bettersizer S3 Plus is an ideal particle analyzer in the food and beverage industry.	Powder Metallurgy	Steel, tin, nickel, copper, aluminum, etc.

Significance

It is crucial to utilize the Bettersizer S3 Plus to measure and control the particle sizes and morphological properties of raw materials in the battery industry because they account for central battery performances, including energy storage, stability, and life cycle.

Storage time, color consistency, flowability, and stability of pigment-based inks resulted from proper controls in the pigment particle shape, size, and size distribution. The Bettersizer S3 Plus characterizes these pigment properties, maximizing final product performances.

The Bettersizer S3 Plus is extremely helpful in industries where quality control standards are exacting, namely the pharmaceutical industry. The particle size and size distributions of both active and inactive ingredients significantly impact drugs' dissolution, body absorption, efficacy, and safety.

The hardening rate, strength, and fluidity of concrete are greatly affected by the particle size distribution of cement. The Bettersizer S3 Plus provides accurate, repeatable, and reliable measurements of cement size and size distribution, increasing the efficiency in the concrete manufacturing process.

The production rates of final powdered particles at the end of the powder metallurgy process are influenced by grains' size and size distribution. Using the Bettersizer S3 Plus to monitor final products' size greatly improves the production efficiency.

Evolutionary Technologies

I - Patented DLOI (Dual Lenses & Oblique Incidence)

System: Laser Diffraction

Laser diffraction technology for routine particle size analysis remains the method of choice across various industrial sectors. The Bettersizer S3 Plus applies the patented DLOI system, which is designed based on the Fourier structure to guarantee the accurate measurement of ultrafine particles from 0.01 µm.

Features & Benefits

- Measures ultrafine particles accurately with the large angular range (0.02 - 165°) with 96 detectors
- Robust optical system with superior resolution using the dual lenses design
- Single short-wave laser system (532 nm) delivers a continuous scattering spectrum with a consistent wavelength
- Zero stabilization and preheating time needed with solid-state light source

II - Dual-Camera System: Dynamic Image Analysis

Dynamic image analysis can strengthen your understanding of materials with comprehensive shape or morphological information that is independent of laser diffraction. Individual particles with specific geometric properties such as agglomerates, crushed particles, and foreign particles can be effectively tracked through the dual-camera system.

Features & Benefits

- 0.5x and 10x cameras photograph extremely wide size range of particles
- High speed strobe lights capture up to **10,000 particle images in 60** seconds, offering authentic shape results
- Suitable for measuring heterogeneous samples with unknown optical properties

III - Groundbreaking Combination: Laser Diffraction with Dynamic Image Analysis

The Bettersizer S3 Plus integrates laser diffraction and dynamic image analysis into one instrument to simultaneously characterize particle size, size distribution, and particle shape over a wide dynamic range. Working in tandem, users can gain a deeper understanding of material behavior to fasten the troubleshooting process and method development process.

Features & Benefits

- 3,500 µm

"The Bettersizer S3 Plus is easy to use and has brought excellent repeatability and high productivity to the research of abrasives."

• DLOI System - precisely measures ultrafine particles down to 0.01 μm • Dual-camera Imaging System - efficiently detects oversized particles up to


• 2-in-1 System - simultaneously obtains particle size and shape results • Fast time-to-result - rapidly generates results in 10 seconds


North University of China

Patented DLOI System

Size Measurement

The Bettersizer S3 Plus achieves exceptional resolution and sensitivity for particle size measurements. The DLOI system allows the size distributions of polydisperse samples to be determined precisely, and the size changes of products to be detected sensitively.

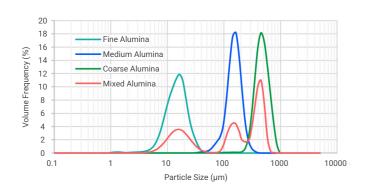




A mixed alumina sample is investigated, and as to be expected, the analysis notes the existence of the three raw samples, suggesting the high-resolution capability of the DLOI system.

The sizes of as-prepared MCC (microcrystalline cellulose) exhibit a slightly decreased trend with the increasing Fe³⁺ concentration, suggesting the highsensitivity capability of the DLOI system. (Adapted from Yue, Xiaopeng, et al. Cellulose 28.3 (2021): 1405-1419.)


Dual-Camera Imaging System

Shape Measurement

An example of additive manufacturing for shape analysis using the Bettersizer S3 Plus is shown below. A representative number of individual particles are recorded from two AlSi10Mg samples, and the number-weighted aspect ratio and circularity are evaluated in compliance with ISO standards. (Adapted from F. Schleife, C. Oetzel. Chem. Ing. Tech. 93.8 (2021): 1199-1203.)



Compared to the fresh powders, the spatter particles show a significantly larger aspect ratio and thus a lower average elongation.

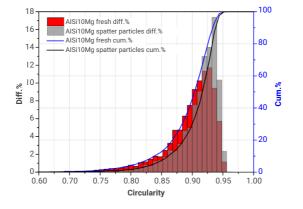

The spatter particles exhibit a higher average circularity and are expected to possess a lower shape anisotropy than the fresh powders.


Combination: Laser Diffraction and Image Analysis

Oversized Particle Detection

Laser diffraction in combination with image analysis can sensitively detect oversized particles that are statistically underrepresented within a wide-distributed sample, such as oversized grains, agglomerates, air bubbles, etc.

An example of an off-specification abrasive is displayed below. The Bettersizer S3 Plus confirms the presence of oversized particles, by showing a size peak at around 120 µm and the images of overly coarse particles.

16



14 0.01

Click to watch the video


Analysis of Samples with Extremely Broad Distributions



Lunar soil analyzed by the Bettersizer S3 Plus


Size Characterization


A very broad distribution of particle size occurs in the range of 0.3 - 516 µm. In the size range of 1 - 10 µm, there is a slow increase, suggesting the presence of a noticeable amount of fine dust.

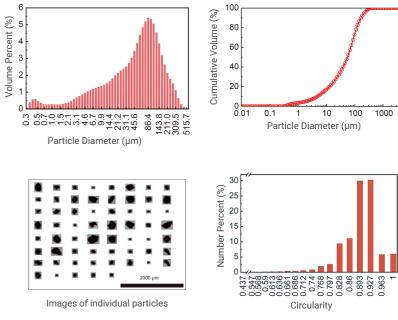

Shape Characterization

The circularity of individual particles of the lunar sample is analyzed based on particle images. Most lunar regolith particles possess high circularity and are thus relatively regular in shape

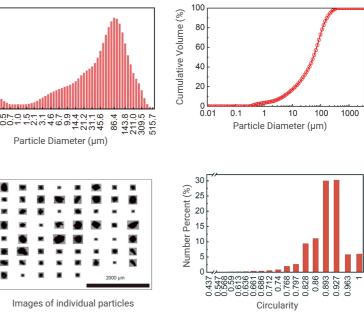

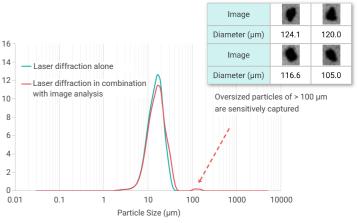

The combined measurement of the Bettersizer S3 Plus is an ideal solution to acquire accurate quantitative results of samples. Here shows an example to measure the soil sample returned from the Moon.

Based on the comprehensive size and shape results, the lunar sample can be described to be well-graded according to geotechnical criteria. (Adapted from Zhang, Hui, et al. Science China Physics, Mechanics & Astronomy 65.2 (2022): 1-8.)

Refractive Index Measurement




No problem. With one simple click, Bettersizer S3 Plus can provide this parameter to you.

Under the Mie theory, measurements by laser diffraction are challenging for samples including:

- · Samples with completely unknown complex refractive index;
- · Samples with heterogeneous chemical composition;
- Samples with significantly different particulate optical properties compared to the bulk material;
- Samples having a distinctly strong optical dispersion (small Abbe number).

Material	Refractive index (literature)	Refractive index (measured)
Carbon black	1.88-0.55i	1.95-0.1i
BaSO ₄	1.65-0.1i	1.71-0.1i
As ₂ O ₃	2.65-0.1i	2.59-0.1i
FeCO ₃	1.875-0.1i	1.83-0.1i
CaCO ₃	(1.53-1.65)-0.1i	1.59-0.1i
SiO ₂	1.54-0.00i	1.57-0.01i

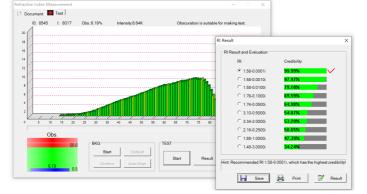

Refractive index measurement is one of

the best solutions. Bettersizer S3 Plus is

· Determine comprehensive refractive index for

Measure samples with unknown properties;

Provide key parameters to calculate particle

· Verify the known data of a material at a

capable of the following:

specific light wavelength;

size distribution in real time.

unknown samples;



BT-A60 Autosampler

Bring Your Productivity to the Next Level

The BT-A60 is a robust, high-throughput autosampler. It measures up to 60 samples in a single run and reduces labor costs while improving laboratory productivity and efficiency. Compatible with the Bettersizer S3 Plus, the BT-A60 provides 24/7 fully automated sample analysis for a variety of analytical applications.

Manual Insertion



- × Skilled operator required
- × Potential risk of human error
- × Risk of cross-contamination
- × Messy workbench
- × Longer sample-to-sample run times

Measurement Automation









- $\sqrt{}$ Save **labor costs**
- $\sqrt{}$ Independent of human error
- $\sqrt{}$ No risk of **cross-contamination**
- √ Well-organized workbench
- $\sqrt{}$ Shorter sample-to-sample run times

Standard Operating Procedure (SOP)

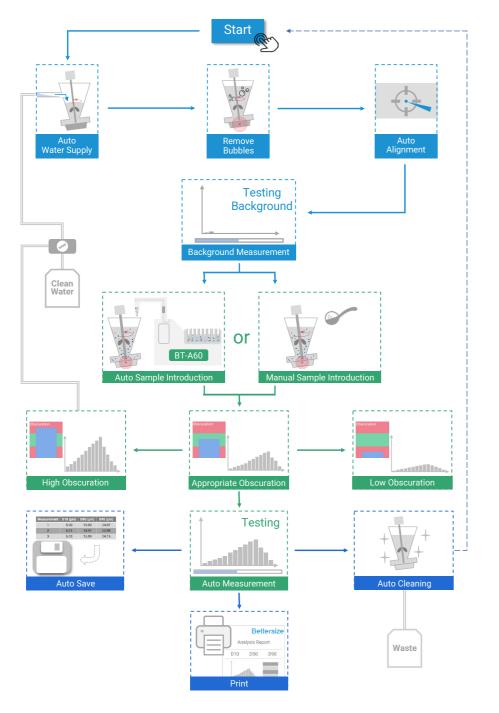


Intuitive and Workflow-oriented Software

The Bettersizer S3 Plus comes with the workflow-oriented software that includes comprehensive built-in functions such as multilingual operating system, signal extraction, system inspection, SOP, etc. Integrated with these functions, the powerful software guarantees the accuracy and repeatability of results.



Template Settings

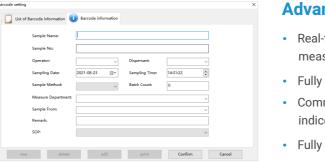

BT-A60Barcode Printing






BT-A60 - A durable, automatic, and high-throughput sampling system designed for automatic measurement for either dry or wet sample.

Autosampler	BT-A60
Measurable Upper Limit	200 µm
Sample Capacity	60 samples
Sampling Volume	0.5 mL - 5 mL



BT-803 Automatic Wet Dispersion Module




Dispersion Module	BT-803
Volume	600 mL
Automation	Fully automated
Compatibility	Samples in aqueous



BT-80N Anti-corrosive Wet Dispersion Module

BT-A60 High-throughtput Autosampler

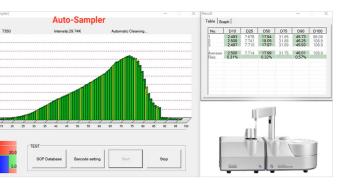

Measurement Interface

Advantages of the software

- Real-time display for determining the optimal measurement conditions
- Fully automatic measurement and cleaning routine
- Commonly used particles and media refractive indices availiable
- Fully comply with 21 CFR Part 11



BT-80N - A solvent-resistant dispersion unit designed for measurements with the organic solvents as the media or where only a small-volume sample is available.


Dispersion Module	BT-80N
Volume	80 mL
Automation	Semi-automated
Compatibility	Samples in organic dispersants

Specification

Dentiale size disatile at an	
Particle size distribution	Suspension, emulsion, dry powders
Particle shape	
eral Deixe in le	
Principle	Laser diffraction and dynamic image technologies
Analysis	Mie scattering theory and Fraunhofer diffraction theory
Typical measurement time	Less than 10 seconds
surement Performance	
Measuring range	0.01 - 3500 μm (Laser System) 2 - 3500 μm (Image System)
Accuracy	<0.5% (NIST certified standards)
Repeatability	<0.5% (NIST certified standards)
Number of size classes	≤100 (adjustable)
Feeding mode	Automatic circulation or semi-automatic circulation
Special functions	Refractive index measurement, SOP settings
Image recognition	Up to 120 fps, up to 10,000 particles per min
Device	
Optical system	Patented DLOI (Dual Lenses & Oblique Incidence) System
Laser	Polarized light-pumped solid-state laser (10 mW / 532 nm)
Detector	96 detectors (forward, lateral and backward arrangements)
Measuring angle	0.02 - 165°
CCD cameras	0.5x and 10x*
Image analysis	1.2 megapixels
ersion Module	
Circulation speed	300 - 2500 r/min
Circulation flow rate	3000 - 8000 mL/min
Ultrasonication	Dry run protection, Max 50 W (adjustable)
Circulation tank capacity	600 mL
vare	
Conformity	21 CFR Part 11, ISO 13320, ISO 13322, USP <429>, CE
Report	Customizable reporting
em Parameters	
Dimensions (L x W x H)	820 × 610 × 290 mm
Weight	48 kg
Voltage	DC 24 V, 50 / 60 Hz, 20 W
puter Configuration (Recommended)	
Computer interface	At least one high-speed USB 2.0 or USB 3.0 port required
Operating system	Windows 7 / Windows 10
Hardware specification	Intel Core i7, 8GB RAM, 500GB HD, two PCI-E X16 interfaces

* The Bettersizer S3 Plus is also available in a single camera (0.5x) model. Contact us for more information.

Global Footprint

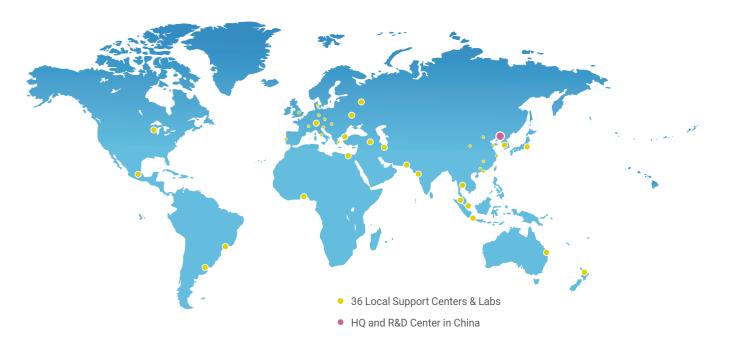

Compliance

All series of Bettersize instruments are in compliance with ISO 9001 and CE certification. The software complies with U.S. FDA 21 CFR Part 11, ensuring the validity and reliability of measurement results and meeting traceability requirements.

FDA U.S. FOOD & DRUG
ADMINISTRATION
13. And and Drug Administration Center for Desizer and Radialogical Health Document Mail Center - MDB-GER 12903 New Research Annual Lines Lines, MC 2009 1000
The sensing is to elementative many of processing strength specific and the processing is to elementative and the processing strength specific and the processi
NAMENDAL DE LA COMPANIA DE LA COMPAN
In advant that follow is somely with COA my defaust may would be sufficient of affected preserve and second my advant of a solid Register of the preserve of the solid second second my advant of Control and Cont
Peace in anarchic the following CDRP Audust Cade() from term anigred to the product() described in this report NO defend as Andphat Warwaring And Defendion Lane Product
If these products will be channel to the United Tables, the strapping locker will used to provide the full PDA Product Cash at the tore of entry, characterized as follows?
HIR-40 DOCUMENT RECENTO, FUED, & ACONOMIDADO
To adorated sufficient from the Orlah Submission Pracess certains general information about the allower stored submission
Accession Transform 2130308-000
Decision Arts, 201
Decement Date: Ad 10, 2021
Indefidences Tanne DANDONG BETTINIZEI INTRUMENTE (70.
Person This submission is a by Janual Report. These Research, Edwards, Lakenstary Laser Products over the period from July 21, 3223 in Jane 83, 3227.
Talamiter Deal Ja
Inst. devide/0001731.com
Reporting Official Naman Na
If you went all allow applicable 750, requirements, you may marked the product() reported. Proce to assee that additional electronic product satisfies carried or medical decises regulations may apply to your product, such as
21 OR 102211, requiring regard supplements under certain circumdances following the same expering forms as used for probabil reports only no finitude.
21 OR 1022 11 requiring around reports to be salestified each year by Daylordize 1 using the appropriate especting form for annual reports
21 OK 1212 - 108, requiring certification to KDA valiation safety performance standards.
21 OYART, repairing manufacturer registration and device liciting, and

Į į	
1 ž	NAC
1 ž	CERTIFICATE OF CONFORMITY OF QUALITY MANAGEMENT SYSTEM
Į.	No. 010000030289 DANDONE BETTERS IZE INSTRUMENTS LTD / NO 000000 BETTERS IZE INSTRUMENTS LTD / NO 000000 BITTERS IZE INSTRUMENTS LTD / NO 000000000000000000000000000000000000
×.	GB/T 19001-2016 / ISO 9001-2015 Standard
Į.	te sonde Millactieiten opwared by this certificate are defined below DEIDLEELEVER AD UNKACUSE OF LEER HETLES SE MALTER ObtRingel Something HetTLES SE ANLTER HETLES ANLYES STELLA DOOR HETLES SE ANLTER HETLES ANLYES STELLA DOOR HETLES SE ANLTER HETLES
N N	Terr of setting of this set If hash from JM 12,2020 to JMM 15,2022 inclusion Northeast Audit Co., Ltd.
×.	te 21-1 elem Rob silver ballingt selend o Tr. Likoving Horingt
ž	
Į	Sortiere auf Frais en road 2 reals for articles and it wind with a solution General Manager Free f
ž	Daz 91 10 2020
×.	× ×
ž	
ž	CNAS
۳.	
×.	No.
V	A 2 4 22 7 4 22 7 4 22 7 12 1 7 22 7 7 22 7 7 12 1

Certified Service and Support

We take great pride in our exceptional customer service, providing excellent application technical support and after-sales service throughout the product life cycle.

From product demonstration and installation, to regular product training and workshops, preventive maintenance programs, software and hardware upgrade, trade-in purchase program, to repair coverage and 24/7 emergency service, our certified service team have you covered.

	CERTIFICATE	Cert No.	086-03-026-00677
Objectively True	of Compliance	Date of leave	15/01/2021
Heider	Dandising Bettersize Instruments No.9 Ganquan Road, Jinquan Indu Province, P. R. China	Ltd. Istrial Park, Dander	g City, Liaoning
Wanufacturer	Dandang Bettersize Instruments No.9 Ganquan Road, Jinquan Indu Province, P. R. China	LML atrial Park, Dandor	g City, Liaoning
Product Description	: Laser Particle Size Analyzer		
Modei(s)	Bettensizer S3 Plus. Bettensizer S3 Bettensizer 5, Bettensizer 25000	Bettersizer ST, Be	ttersizer 50.
Requirements and Standard(s)	: Low Voltage Drective 2014/35/EU Electromagnetic Compatibility 201- EN 61310-1 2010 EN 61325-1 2013	NISOED	
Report No.	086-03-011-04789		
Date of Expiry	2610/2025		
certifies that the above in also the Technical File, h	CHMSCHE BEWERTUNG S.A. as intrioned products were witnessed to as been received, archived and proce- rical File is adequate in respect with th ments and standard(s).	y us during testing red to the fullness r	when applicable, an examination by us an
certifies that the above n also the Technical File, h we confirm that the Techn above mentioned require This Certificate is assed in time and place only for the	tertioned products were witnessed to as been necelved, anthrived and proop incal File is adequate in respect with th ments and standard(s), conjunction with the above mentioned Re product and configuration described her	y us during testing ed to the fulness of the basic health and sport and reflects find	when applicable, an examination by us an safety prerequisites in ings during inspection in
certifies that the above n also the Technical File, h we confirm that the Techni above mentioned requires - The Certificate is issued in time and place only for the how their contractual regs	settioned products were witnessed to as been nooked, archived and prior scal File is adequate in respect with th ments and standard(s), conjunction with the above mentioned Re is product and configuration described her mabilities.	y us during testing red to the fulness a re basic health and sport and reflects find sty and does not rel	when applicable, an examination by us an safety prerequisites i lings during inspection i nese buyer and/or sele
certifies that the above n also the Technical File, h we confirm that the Techni above mentioned requires - The Certificate is issued in time and place only for the how their contractual regs	tertioned products were witnessed to as been necelved, anthrived and proop incal File is adequate in respect with th ments and standard(s), conjunction with the above mentioned Re product and configuration described her	y us during testing red to the fulness a re basic health and sport and reflects find sty and does not rel	when applicable, an examination by us an safety prerequisites i lings during inspection i nese buyer and/or sele
certifies that the above n also the Technical File, th we confirm that the Technisons above mentioned requires The Certificate is issued in time and piece only for the from their contractual rega- All modifications to the Te affectation. The CE marking can be us	settioned products were witnessed to as been nooked, archived and prior scal File is adequate in respect with th ments and standard(s), conjunction with the above mentioned Re is product and configuration described her mabilities.	y us during testing red to the fulness is re basic health and sport and reflects fina rity and does not rel wr Company to ensu- scherer, after completi-	when applicable, an examination by us an safety prerequisites in ings during inspection i ease byper and/or actor re further validity of the re further validity of the rest.
certifies that the above in also the Technical File, h we confirm that the Techni above mentioned require in the Certificate a lawed in them there contractual reaso All modifications to the Te absorbtion. The Off marking can be as of Conformity and compile The certificate of compiler	tentitional products were witnessen bit ab been received, activited and propo- tical File is adequate in respect with the ments and standard(s). Comparison with advome metaloaid A product and configuration devoted her mobilies. United File indust be find submitted to c and, under the responsibility of the mean- tim with responsibility of the mean- tim with environment (2) standards and regular on with means of the responsibility of the mean-	y us during testing red to the fullness is to basic health and sport and reflects find rety and does not red will Company to ansu- sclurer, after company fons.	when applicable, an exemination by us an safety prerequisites i legs during inspection i nace buyer and/or solu or of an EC Declarato transferb, and does no
certifies that the above n also the Tachnical File, th we confirm that the Tachni above mentioned requires - The Certificate is asset in them their contractual regu- - Ar modifications to the Te assession. - The CE marking can be as of Contently and complia- tion certificate of complia- modestie in Alother Body.	terificited products were whreesed to achieve the advectory achieves and the tical File is advectory in the advectory with the method and advectory achieves and compared and configuration described her product and configuration described her advectory and the responsement of the confidence under Col selections of col- metications and the responsement of the confidence under Col selection act on confidence under Col selections of the confidence under Col selection act on confidence under Col selection act on confidence under Col selections act on confidence under Col selections act on confidence under Col selections act on	y us during testing red to the fullness is to basic health and sport and reflects find rety and does not red will Company to ansu- sclurer, after company fons.	when applicable, an exemination by us an safety prerequisites i legs during inspection i nace buyer and/or solu or of an EC Declarato transferb, and does no
certifies that the above n also the Tachnical File, th we confirm that the Tachni above mentioned requires - The Certificate is asset in them their contractual regu- - Ar modifications to the Te assession. - The CE marking can be as of Contently and complia- tion certificate of complia- modestie in Alother Body.	tentitional products were witnessen bit ab been received, activited and propo- tical File is adequate in respect with the ments and standard(s). Comparison with advome metaloaid A product and configuration devoted her mobilies. United File indust be find submitted to c and, under the responsibility of the mean- tim with responsibility of the mean- tim with environment (2) standards and regular on with means of the responsibility of the mean-	y us during testing red to the fullness is to basic health and sport and reflects find rety and does not red will Company to ansu- sclurer, after company fons.	when applicable, an exemination by us an safety prerequisites i legs during inspection i nace buyer and/or solu or of an EC Declarato transferb, and does no
certifies that the above in above The Technica File, h are confirm that the Techni- table and the technica File and the technical in a second of the technical in a second the technical in a second technical technical in a second technical and technical technical and technical technical and technical technical and technical technical technical and technical te	setting products were wheneved to that if his a despace in respect with the product of the solar method of the origination of the solar method with comparison of the solar method with a solar transmission of the method. The should be the solariset to a solar the solar that and the solar solar transmission of and under the responsibility of the neutron and solar the responsibility of the solar theory is the responsibility of the solar theory is the resolution. The solar theory is the resolution of the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is theory is the solar theory is the solar theory is the resolution of the solar theory is the solar theory is theory is theory is	y us during techniques o les basic health and sport and reflects fra thy and dises nor nel wr Company to ansu- sciawr, aftwr compati- fices. a show mentioned o a show mentioned o	when applicable, an safety prevauities i safety prevauities i inge suring impaction mean buyer and/or sold on of an EC Destantio candrates and store re at the request of to at the request
certifies that the above in a data of the Technical File, it was confirm that the Technical File, it was confirmed requires the technical file of the second places only for the technical response of technical respons	setting products were wheneved to that if his a despace in respect with the product of the solar method of the origination of the solar method with comparison of the solar method with a solar transmission of the method. The should be the solariset to a solar the solar that and the solar solar transmission of and under the responsibility of the neutron and solar the responsibility of the solar theory is the responsibility of the solar theory is the resolution. The solar theory is the resolution of the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is the solar theory is the resolution of the solar theory is theory is the solar theory is the solar theory is the resolution of the solar theory is the solar theory is theory is theory is	y us during testing and to the fulness + is basic health and sport and reflects find and date nor rel wr Company to ansu- scurer, after somplets associated a above mentioned / a volumery control	when applicable, an safety prevauities i safety prevauities i inge suring impaction mean buyer and/or sold on of an EC Destantio candrates and store re at the request of to at the request





www.bettersizeinstruments.com info@bettersize.com

Bettersize Instruments Ltd.

Address: No. 9, Ganquan Road, Jinquan Industrial Park, Dandong, Liaoning, China Postcode: 118009 Tel: +86-415-6163800 Fax: +86-415-6170645

Bettersize Inc.

Address: Suite K-2, 3188 Airway Ave, Costa Mesa, CA 92626, United States Tel: 833-699-7493(SIZE) Visit Our Bettersizer S3 Plus Site:



Visit Our Official Youtube Channel:



Disclaimer: By using or accessing the brochure, you agree with the Disclaimer without any qualification or limitation. Diligent care has been used to ensure that the information in this brochure is accurate, Bettersize instruments Ltd. shall not be liable for errors contained herein or for damages in connection with the use of this material. The information on this brochure is presented as general information and no representation or warranty is expressly or impliedly given as to its accuracy, completeness or correctness. It does not constitute part of a legal offer or contract. Bettersize Instruments Ltd. reserves the right to modify, alter, add and delete the content outlined in the brochure without prior notice and without any subsequent liability to the company.

Copyright: © 2023 Bettersize Instruments Ltd. | All Rights Reserved